




## Phonak Naída P-UP (P90/P70/P50/P30/Trial)


### HE11 2 cm<sup>3</sup> coupler data

ANSI / ASA S3.22-2014  
IEC 60118-0 : 2015

#### Output sound pressure level

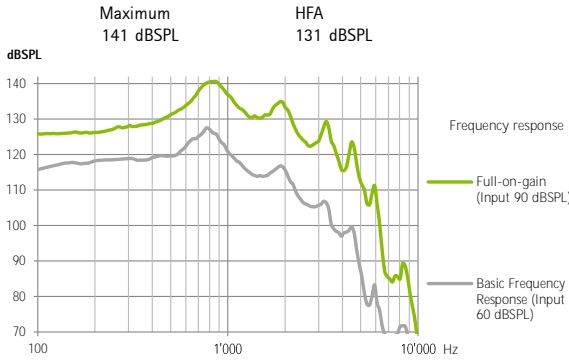


#### Acoustic gain

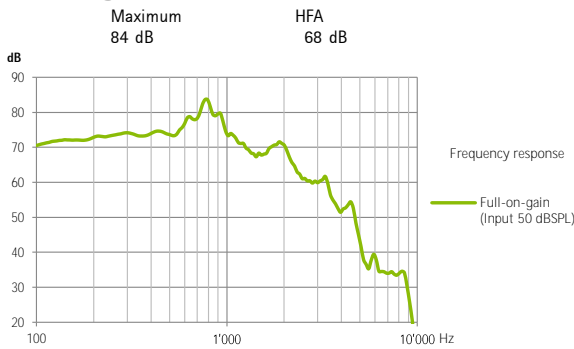

Frequency range	<100 Hz - >4700 Hz			
Total harmonic distortion	500 Hz	800 Hz	1600 Hz	3200 Hz
	5.0%	1.0%	1.0%	1.0%
Battery current	3.3 mA			
Equivalent input noise level	19 dBSPL			


#### Induction coil sensitivity

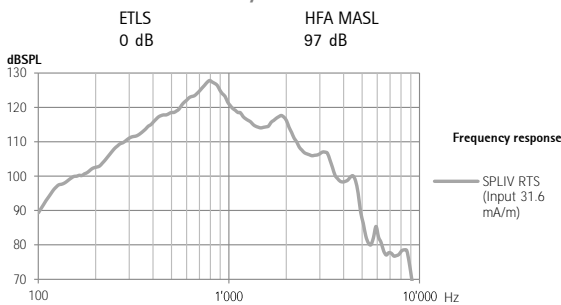


### HE11 680 2 cm<sup>3</sup> coupler data

ANSI / ASA S3.22-2014  
IEC 60118-0 : 2015

#### Output sound pressure level

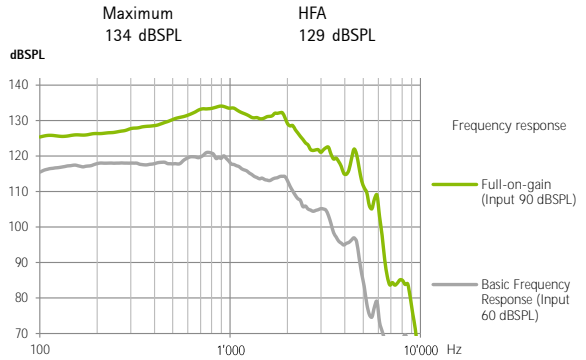


#### Acoustic gain

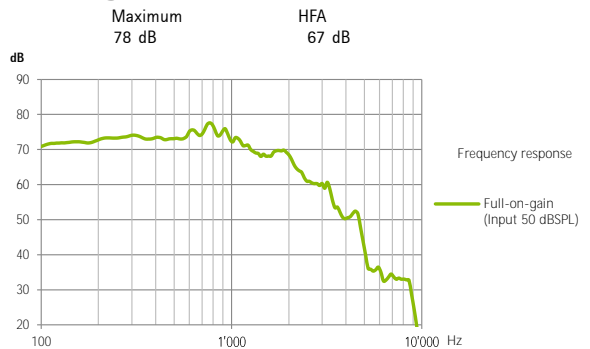

Frequency range	<100 Hz - >4700 Hz			
Total harmonic distortion	500 Hz	800 Hz	1600 Hz	3200 Hz
	3.0%	1.0%	1.0%	1.0%
Battery current	2.8 mA			
Equivalent input noise level	19 dBSPL			

#### Induction coil sensitivity

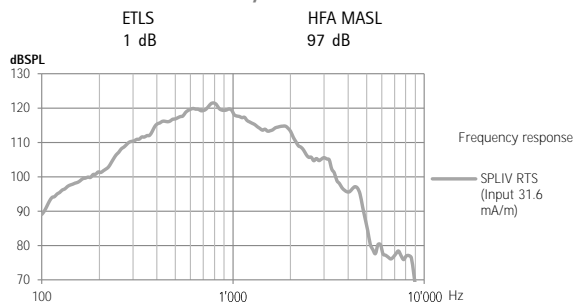

#### General test information

- Supply voltage 1.3 V / impedance 3.3 Ω
- Specific measurement settings are used: RTS adjustment with volume control.
- The device is operating in linear mode
- Low-level expansion is active
- All data obtained are measured with Phonak Target measurement settings

#### Warnings

- ⚠ This hearing aid has an output sound pressure level that can exceed 132 dB SPL. Special care should be taken when fitting this instrument as there is a risk of impairing the residual hearing of the user.
- ⚠ Changes or modifications to the hearing aid that are not explicitly approved by the manufacturer are not permitted. Such changes may damage the ear or the hearing aid.